

This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

As rescanning documents *will not* correct images,
please do not report the images to the
Image Problem Mailbox.

THIS PAGE BLANK (USPTO)

(19) World Intellectual Property Organization
International Bureau




(43) International Publication Date
16 May 2002 (16.05.2002)

PCT

(10) International Publication Number
WO 02/38052 A2

- (51) International Patent Classification⁷: **A61B 17/00**
- (21) International Application Number: **PCT/EP01/12243**
- (22) International Filing Date: **23 October 2001 (23.10.2001)**
- (25) Filing Language: **English**
- (26) Publication Language: **English**
- (30) Priority Data:
09/709,087 **10 November 2000 (10.11.2000)** **US**
- (71) Applicant (*for all designated States except US*): **BOSTON SCIENTIFIC LIMITED** [IE/BB]; Financial Services Centre, P.O. Box 111, Bishop's Court Hill, St. Michael (BB).
- (72) Inventors; and
- (75) Inventors/Applicants (*for US only*): **JENKINS, Thomas, R.** [US/US]; 3750 McClelland Ave., Oakland, CA 94619 (US). **SWANSON, David, K.** [US/US]; 1458 Ridgeley Drive, Campbell, CA 94040 (US).
- (74) Agent: **VIERING, JENTSCHURA & PARTNER**; Steinsdorfstr. 6, 80538 Munich (DE).
- (81) Designated States (*national*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, PH, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, TZ, UA, UG, US, UZ, VN, YU, ZA, ZW.
- (84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).
- Published:
— *without international search report and to be republished upon receipt of that report*
- For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.*

(54) Title: **STEERABLE LOOP STRUCTURES FOR SUPPORTING DIAGNOSTIC AND THERAPEUTIC ELEMENTS IN CONTACT WITH BODY TISSUE**

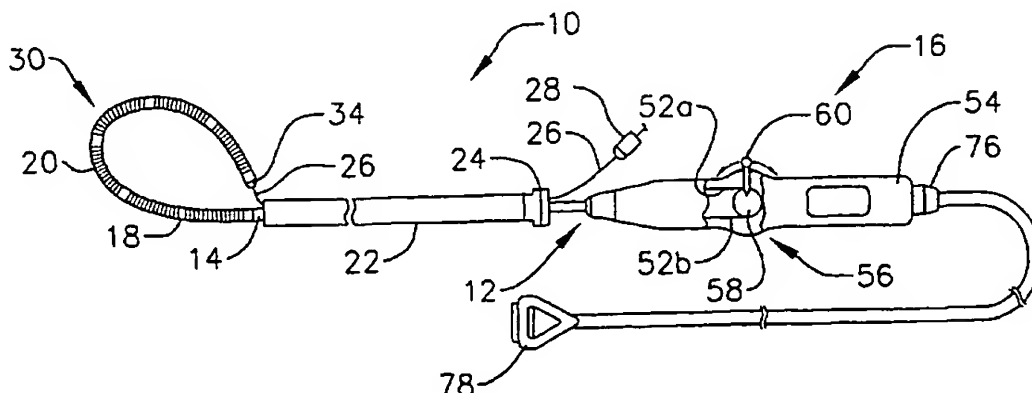

(57) Abstract: A probe that includes an elongate body (12) and a steerable loop structure (30, 74) that supports electrodes (20) or other operative elements against the body tissue.



WO 02/38052 A2

STEERABLE LOOP STRUCTURES FOR SUPPORTING DIAGNOSTIC AND THERAPEUTIC ELEMENTS IN CONTACT WITH BODY TISSUE

BACKGROUND OF THE INVENTIONS

1. Field of Inventions

The present inventions relate generally to medical devices that support one or more diagnostic or therapeutic elements in contact with body tissue and, more particularly, to loop structures that support one or more diagnostic or therapeutic elements in contact with body tissue.

2. Description of the Related Art

There are many instances where diagnostic and therapeutic elements must be inserted into the body. One instance involves the treatment of cardiac conditions such as atrial fibrillation and atrial flutter which lead to an unpleasant, irregular heart beat, called arrhythmia.

Normal sinus rhythm of the heart begins with the sinoatrial node (or "SA node") generating an electrical impulse. The impulse usually propagates uniformly across the right and left atria and the atrial septum to the atrioventricular node (or "AV node"). This propagation causes the atria to contract in an organized way to transport blood from the atria to the ventricles, and to provide timed stimulation of the ventricles. The AV node regulates the propagation delay to the atrioventricular bundle (or "HIS" bundle). This coordination of the electrical activity of the heart causes atrial systole during ventricular diastole. This, in turn, improves the mechanical function of the heart. Atrial fibrillation occurs when anatomical obstacles in the heart disrupt the normally uniform propagation of electrical impulses in the atria. These anatomical obstacles (called "conduction blocks") can cause the electrical impulse to degenerate into several circular wavelets that circulate about the obstacles. These wavelets, called "reentry circuits," disrupt the normally uniform activation of the left and right atria.

Because of a loss of atrioventricular synchrony, the people who suffer from atrial fibrillation and flutter also suffer the consequences of impaired

hemodynamics and loss of cardiac efficiency. They are also at greater risk of stroke and other thromboembolic complications because of loss of effective contraction and atrial stasis.

One surgical method of treating atrial fibrillation by interrupting pathways for reentry circuits is the so-called "maze procedure" which relies on a prescribed pattern of incisions to anatomically create a convoluted path, or maze, for electrical propagation within the left and right atria. The incisions direct the electrical impulse from the SA node along a specified route through all regions of both atria, causing uniform contraction required for normal atrial transport function. The incisions finally direct the impulse to the AV node to activate the ventricles, restoring normal atrioventricular synchrony. The incisions are also carefully placed to interrupt the conduction routes of the most common reentry circuits. The maze procedure has been found very effective in curing atrial fibrillation. However, the maze procedure is technically difficult to do. It also requires open heart surgery and is very expensive.

Maze-like procedures have also been developed utilizing catheters which can form lesions on the endocardium (the lesions being 1 to 15 cm in length and of varying shape) to effectively create a maze for electrical conduction in a predetermined path. The formation of these lesions by soft tissue coagulation (also referred to as "ablation") can provide the same therapeutic benefits that the complex incision patterns that the surgical maze procedure presently provides, but without invasive, open heart surgery.

Catheters used to create lesions typically include a relatively long and relatively flexible body portion that has a soft tissue coagulation electrode on its distal end and/or a series of spaced tissue coagulation electrodes near the distal end. The portion of the catheter body portion that is inserted into the patient is typically from 23 to 55 inches (58.4 to 139.7 cm) in length and there may be another 8 to 15 inches (20.3 to 38.1 cm), including a handle, outside the patient. The length and flexibility of the catheter body allow the catheter to be inserted into a main vein or artery (typically the femoral artery), directed into the interior of the heart, and then manipulated such that the coagulation

electrode contacts the tissue that is to be ablated. Fluoroscopic imaging is used to provide the physician with a visual indication of the location of the catheter.

5 In some instances, the proximal end of the catheter body is connected to a handle that includes steering controls. Exemplary catheters of this type are disclosed in U.S. Patent No. 5,582,609. In other instances, the catheter body is inserted into the patient through a sheath and the distal portion of the catheter is bent into loop that extends outwardly from the sheath. This may be accomplished by pivotably securing the distal end of the catheter to the distal
10 end of the sheath, as is illustrated in U.S. Patent No. 6,071,279. The loop is formed as the catheter is pushed in the distal direction. The loop may also be formed by securing a pull wire to the distal end of the catheter that extends back through the sheath, as is illustrated in U.S. Patent No. 6,048,329. Loop catheters are advantageous in that they tend to conform to different tissue
15 contours and geometries and provide intimate contact between the spaced tissue coagulation electrodes (or other diagnostic or therapeutic elements) and the tissue. Loop catheters also tend to cause the atria to conform to the shape of the loop.

20 The inventor herein has determined that one issue associated with conventional catheters is that, when deployed, the loop structures tend to follow the path of least resistance and occupy the largest diameter portion of the atria. The largest diameter portion is not, however, always the intended diagnostic or therapeutic location. This is especially true in those instances where the preferred loop position is near an atrial appendage or a ventricular
25 annulus because conventional loop structures can slip into the atrial appendage or ventricular annulus.

Accordingly, the inventor herein has determined that a need exists generally for loop structures that can be deployed within the atrium (or some other bodily structure) and, if desired, deflected in such a manner that they
30 occupy a portion of the atrium other than the largest diameter portion.

SUMMARY OF THE INVENTION

Accordingly, the general object of the present inventions is to provide a device that avoids, for practical purposes, the aforementioned problems. In particular, one object of the present inventions is to provide a loop structure that can, if desired, be deployed with a bodily structure in such a manner that it occupies a portion of the bodily structure other than the largest diameter portion and/or the portion associated with the path of least resistance. Another object of the present inventions is to provide a loop structure having at least a portion that can, if desired, be deflected.

In order to accomplish some of these and other objectives, a probe in accordance with one embodiment of a present invention includes an elongate body that can be deployed as a loop and a steering element secured to the distal portion of the elongate body. When the loop is deployed in a loop plane, for example, the steering element may be used to deflect a portion of the loop out of the loop plane. Such a probe advantageously allows the physician to steer the loop into contact with intended diagnostic and therapeutic locations which the loop would not contact absent such steering. In an atrium, for example, the steering capability may be used by a physician to move a portion of the loop away from an atrial appendage located along the path of least resistance to a more desirable location.

The above described and many other features and attendant advantages of the present inventions will become apparent as the inventions become better understood by reference to the following detailed description when considered in conjunction with the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

Detailed description of preferred embodiments of the inventions will be made with reference to the accompanying drawings.

Figure 1 is a side view of a catheter in accordance with a preferred embodiment of a present invention.

Figure 2 is a section view of the distal end of the exemplary catheter illustrated in Figure 1.

Figure 3 is a top view of the distal region of the exemplary catheter illustrated in Figure 1.

Figure 4 is a section view of a portion of the distal region of the exemplary catheter illustrated in Figure 1.

5 Figure 5 is a section view of another portion of the distal region of the exemplary catheter illustrated in Figure 1.

Figure 6 is a top view of the distal region of the exemplary catheter illustrated in Figure 1 with a portion steered out of the loop plane.

10 Figure 7 is an end view of the distal region of the exemplary catheter illustrated in Figure 1 with a portion steered out of the loop plane.

Figure 8 is a top view of the distal region of another catheter in accordance with another preferred embodiment of a present invention with a portion steered out of the loop plane.

15 Figure 9 is an end view of the exemplary catheter illustrated in Figure 8.

Figure 10 is a side view of the distal region of a catheter in accordance with still another preferred embodiment of a present invention.

20 Figure 11 is a side view of the distal region of a catheter in accordance with yet another preferred embodiment of a present invention with some of the electrodes shown in phantom lines for clarity.

Figure 12 is a section view taken along line 12-12 in Figure 11.

Figure 13 is a section view taken along line 13-13 in Figure 11.

Figure 14 is an end view of the distal member in the exemplary catheter illustrated in Figure 11.

25 Figure 15 is a section view taken along line 15-15 in Figure 11.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

30 The following is a detailed description of the best presently known modes of carrying out the inventions. This description is not to be taken in a limiting sense, but is made merely for the purpose of illustrating the general principles of the inventions.

The detailed description of the preferred embodiments is organized as follows:

- I. Introduction
- II. Steerable Loop Structures
- 5 III. Electrodes, Temperature Sensing and Power Control

The section titles and overall organization of the present detailed description are for the purpose of convenience only and are not intended to limit the present inventions.

I. Introduction

10 The present inventions may be used within body lumens, chambers or cavities for diagnostic or therapeutic purposes in those instances where access to interior bodily regions is obtained through, for example, the vascular system or alimentary canal and without complex invasive surgical procedures. For example, the inventions herein have application in the diagnosis and
15 treatment of arrhythmia conditions within the heart. The inventions herein also have application in the diagnosis or treatment of ailments of the gastrointestinal tract, prostate, brain, gall bladder, uterus, and other regions of the body.

With regard to the treatment of conditions within the heart, the present
20 inventions are designed to produce intimate tissue contact with target substrates associated with various arrhythmias, namely atrial fibrillation, atrial flutter, and ventricular tachycardia. For example, embodiments of the present inventions, which may include diagnostic and/or soft tissue coagulation electrodes, can be used to map tissue and/or create lesions in tissue that cure
25 arrhythmias.

Although the present inventions are discussed primarily in the context of catheter-based probes, the inventions are also adaptable for use with probes other than catheter-based probes. For example, the structures disclosed herein may be used in conjunction with hand held surgical devices
30 (or "surgical probes"). The distal end of a surgical probe may be placed directly in contact with the targeted tissue area by a physician during a surgical procedure, such as open heart surgery. Here, access may be

obtained by way of a thoracotomy, median sternotomy, or thoracostomy. Exemplary surgical probes are disclosed in U.S. Patent No. 6,071,281.

Surgical probe devices in accordance with the present inventions preferably include a handle, a relatively short shaft, and one of the distal assemblies described hereafter in the catheter context. Preferably, the length of the shaft is about 4 inches to about 18 inches (10.2 to 45.7 cm). This is relatively short in comparison to the portion of a catheter body that is inserted into the patient (typically from 23 to 55 inches (58.4 to 139.7 cm) in length) and the additional body portion that remains outside the patient. The shaft is also relatively stiff. In other words, the shaft is either rigid, malleable, or somewhat flexible. A rigid shaft cannot be bent. A malleable shaft is a shaft that can be readily bent by the physician to a desired shape, without springing back when released, so that it will remain in that shape during the surgical procedure. Thus, the stiffness of a malleable shaft must be low enough to allow the shaft to be bent, but high enough to resist bending when the forces associated with a surgical procedure are applied to the shaft. A somewhat flexible shaft will bend and spring back when released. However, the force required to bend the shaft must be substantial.

II. Steerable Loop Structures

As illustrated for example in Figures 1 and 2, a catheter 10 in accordance with a preferred embodiment of a present invention includes a hollow, flexible catheter body 12 that is preferably formed from two tubular parts, or members. The proximal member 14 is relatively long and is attached to a handle 16, while the distal member 18, which is relatively short, carries a plurality of spaced electrodes 20 or other operative elements. The proximal member 14 is typically formed from a biocompatible thermoplastic material, such as a Pebax® material (polyether block emide) and stainless steel braid composite, which has good torque transmission properties. In some implementations, an elongate guide coil (not shown) may also be provided within the proximal member 14. The distal member 18 is typically formed from a softer, more flexible biocompatible thermoplastic material such as unbraided Pebax® material, polyethylene, or polyurethane. The proximal and distal

members, which are about 5 French to about 9 French (1.66 mm to 3 mm) in diameter, are preferably either bonded together with an overlapping thermal bond or adhesively bonded together end to end over a sleeve in what is referred to as a "butt bond."

5 The catheter 10 is used in combination with a sheath 22, which preferably has a greater inherent stiffness than the distal region of the catheter 12 (i.e. the distal member 18, the electrodes 20 and a spline 32 that is discussed below with reference to Figures 4 and 5). The sheath 22 should also be lubricious to reduce friction during movement of the catheter body 12.

10 With respect to materials, the sheath 14 is preferably a Pebax® and stainless steel braid composite. Other materials, such as polytetrafluoroethylene (PTFE), can also be used. The wall thickness of the sheath 22 is preferably about 0.013 inch (3.3 mm), which will not add significantly to the overall thickness of the catheter 10. A handle 24, which is preferably in the form of a

15 hemostatic connector that can be used to fix the relative positions of the catheter 12 and sheath 22, is mounted on the proximal end of the sheath.

 In the exemplary embodiment illustrated in Figure 1, the distal end of the sheath 22 is perpendicular to the longitudinal axis of the sheath. However, the distal end of the sheath 22 may also be cut at an angle and tapered in a

20 transverse direction relative to the longitudinal axis of the sheath to effect the shape loop formed by the distal region of the catheter 12.

 A pull wire 26 extends from the distal end of the catheter 12 through the sheath 22 in the exemplary embodiment illustrated in Figure 1. The proximal end of the pull wire 26 includes an adjustable stop/handle 28. The

25 pull wire 26 is preferably a flexible, inert cable constructed from strands of metal wire material, such as Nickel Titanium (commercially available under the trade name Nitinol®) or 17-7 stainless steel, that is about 0.012 to 0.018 inch (0.30 to 0.46 mm) in diameter. Alternatively, the pull wire 26 may be formed from a flexible, inert stranded or molded plastic material. The pull wire

30 26 is also preferably round in cross-section, although other cross-sectional configurations can be used.

Holding the handle 28 stationary, the physician deploys a loop structure 30 by advancing the catheter body 12 through the sheath 22. Once the loop structure 30 has been formed, the physician can pull on the wire 26 to decrease the exposed length of the pull wire beyond the distal end of the sheath 22. Further adjustments to the loop may be made by advancing or retracting the catheter body 12 within the sheath 22 or by putting tension on the pull wire 24. For example, a portion of the loop structure 30 may be bent out of the loop plane. This aspect of the invention is discussed in greater detail below with reference to Figures 5-9. In addition, the loop structure 30 can be rotated by rotating the catheter body 12 with its handle 16.

As illustrated in Figures 2 and 4, the exemplary catheter body 12 also includes a flexible spline (or "core wire") 32. The flexible spline 32 is preferably a wire having a diameter of approximately 0.023 inch (0.58 mm) that is positioned inside of and passes within the length of the catheter body 12. The flexible spline 32 is fixedly secured to the handle 16 at the proximal end of the catheter body 12 and to a tip member 34 in the manner described below. The tip member 34 is in turn secured to the distal end of the catheter body 12 with adhesive. In the preferred embodiment, the flexible spline 32 is made from resilient, inert wire, such as Nitinol® material or 17-7 stainless steel. Resilient injection molded plastic can also be used. The exemplary spline 32 is round in cross section, although other cross sectional configurations can be used. The flexible spline 32 may, if desired, also have a preset curvature accomplished by thermally presetting the spline at 500°C for 8 minutes. The super-elastic properties of the material should, however, be maintained.

Referring more specifically to Figures 1, 3 and 4, the flexible spline 32 includes a flattened portion 36, which is preferably adjacent to (i.e. either just proximal to, just distal to, or aligned with) the proximal end of the distal member 18, that allows this portion of the flexible spline to be bent with less force than would otherwise be required. The flattened portion 36 also causes the distal member 18 to bend, and the loop structure 30 to be formed, in a flat loop plane (note the side view in Figure 1 and the top view in Figure 3). In an

embodiment where the flexible spline 32 has a diameter of approximately 0.023 inch (0.58 mm), the thickness of the flattened portion 36 would be about 0.018 inch (0.46 mm) and the length would be about 1.75 inches (4.45 cm).

The flexible spline 32 may also be used to anchor the pull wire 26. As illustrated for example in Figure 2, the distal end 38 of the flexible spline 32 is fixedly engaged in an in-line manner to the end 40 of the pull wire 26 with a stainless steel crimp tube 42. The in-line connection of the flexible spline 32 and pull wire 26 allows for a reduction in the overall diameter of distal portion of the catheter body 12. This provides a significant clinical advantage over devices having side by side pull wire connections which create a larger diameter device. The pull wire 26 passes through a pull wire bore 44 in the catheter tip member 24 and through a bore 46 in the distal end of the crimp tube 42.

The tip member 34 is preferably formed from platinum-iridium (90/10) and is fixedly engaged with, for example, silver solder, adhesive or spot welding, to the distal end of crimp tube 42. The flexible spline 32 is preferably electrically insulated with a thin walled polyester heat shrink tube 48 that extends beyond the proximal end of the crimp tube 42. Other pull wire configurations, other methods of attaching the pull wire to the catheter body, and methods of reducing stress on the pull wire are disclosed in U.S. Patent No. 6,048,329.

The exemplary catheter 10 present also includes a loop deflection system that allows the physician to steer a portion 50 of the loop structure 30 out of the loop plane in the manner illustrated in Figures 6 and 7.

As illustrated in Figures 1 and 5, the steering capability may, for example, be provided through the use of one or more steering wires. The exemplary catheter 10 includes a pair of steering wires 52a and 52b which pass through the heat shrink tube 48 and are secured to the flexible spline 32 with a crimp joint, solder, adhesive or other suitable instrumentalities. Steering wires 52a and 52b extend proximally to the exemplary handle 16, which includes handle body 54 and a steering assembly 56 that consists of a cam wheel 58 and a lever 60. The proximal ends of each of the steering wires 52a

and 52b are secured to a cam wheel 58. Tension is applied to steering wire 52a wire by urging the lever 60 proximally, while tension is applied to the steering wire 52b by urging the lever distally. Portion 50 in Figures 6 and 7 has been steered out of the loop plane by moving the lever in the clockwise direction and can be steered in the opposite direction by moving the lever in the counter-clockwise direction. Additional information concerning this type of handle is disclosed in U.S. Patent No. 5,636,634. Other types of handles, such as piston and cylinder style handles, may also be employed.

The steering of portion 50 may be facilitated by forming a second flattened portion 62 in the spline 32 just proximally of the point at which the steering wires 52a and 52b are attached to the spline. The second flattened portion 62, which is rotated 90 degrees relative to the flattened portion 36, facilitates the steering of portion 50 by giving the bend directionality and creating a live hinge. In an embodiment where the flexible spline 32 has a diameter of approximately 0.023 inch (0.58 mm), the thickness of the second flattened portion 62 would be about 0.010 inch (0.25 mm) and the length would be about 0.50 inch (1.27 cm).

In an alternative embodiment, which is especially useful in situations that require a greater portion of the loop to be steered out of the loop plane, is illustrated in Figures 8 and 9. Steerable portion 50' is larger than the steerable portion 50 illustrated in Figures 6 and 7 because the second flattened portion (not shown) in the embodiment illustrated in Figure 8 and 9 is longer than the second flattened portion 62 illustrated in Figure 5. Here, a suitable length for the second flattened portion 62 in an embodiment where the flexible spline 32 has a diameter of approximately 0.023 inch (0.58 mm) would be about 1.5 inches (3.81 cm).

The present inventions are also applicable to loop catheters in which the distal portion of catheter body is connected to the distal portion of the sheath. As illustrated for example in Figure 10, the exemplary catheter 64 does not include a pull wire and instead is used in combination with a sheath 66 which has a distal member 68 that is connected to the distal end of the catheter 64. A slot is formed in the distal portion of the sheath 66 and the

remnant 70 forms a flexible joint. A stiffening element 72 may also be provided. The loop 74 is formed when the catheter 64 is urged distally relative to the sheath 66, thereby causing the distal portion of the catheter to bulge outwardly in the manner illustrated in Figure 10. Although not shown in Figure 10, exemplary catheter 64 also includes the loop steering elements described above.

The loop steering elements described above may also be used in other loop catheters where the distal portion of catheter body is connected to the distal portion of the sheath. One example is a catheter wherein the distal end of the catheter body is connected to the distal end of a sheath by a short wire. This and other examples of such loop catheters are disclosed in U.S. Patent No. 6,071,274.

In another alternative embodiment, and as illustrated for example in Figures 11-15, the steering wires 52a and 52b may be secured at respective points on the exterior of the catheter and then directed to respective points that are on the opposite side of the catheter. Such an arrangement provides more steering torque than would be realized if the steering wires were simply allowed to extend proximally from their attachment point in the manner illustrated in Figure 5 because the present arrangement increases the effective lever length. This arrangement is also applicable to steerable catheters that are not adapted to be bent into loops as well as catheters with a single steering wire, whether adapted to be bent into a loop or not.

The exemplary catheter 84 illustrated in Figures 11-15 is in many respects identical to the catheter 10 illustrated in Figures 1-7. Here, however, the steering wires 52a and 52b are not secured to the spline 32. The steering wires 52a and 52b are instead directed through steering wire lumens 86a and 86b which are formed in the distal member 18'. The steering wire lumens 86a and 86b, which include respective inlets 88a and 88b and outlets 90a and 90b, each wind half way (i.e. 180 degrees) around the distal member 18'. The rotational position change measured as a function of longitudinal position change is preferably constant from one end of the steering wire lumens 86a and 86b to the other. Referring more specifically to Figure 15, the inlets 88a

and 88b and outlets 90a and 90b are also perpendicular to (i.e. offset 90 degrees from) the flattened surfaces of the second flattened portion 62. Although the exemplary distal member 18' could be formed by a multi-lumen extrusion process so if desired, the preferred process is a molding process. Here, core pins formed from flexible metal tubes could be used to form the steering wire lumens 86a and 86b.

The distal ends of the steering wires 52a and 52b extend outwardly through the outlets 90a and 90b and are secured to one of the electrodes 20 by, for example, welding or soldering. Alternatively, the steering wires 52a and 52b could be secured to a support ring (not shown) mounted on the exterior of the distal member 18'. A guide coil (not shown), or other tubular member through which the steering wires 52a and 52b would pass, may be positioned within the steering wire lumens 86a and 86b to provide additional column strength.

In an alternative implementation, the steering wire lumens 86a and 86b would be eliminated and replaced by channels formed in the outer surface of the distal member 18'. The channels would extend around the distal member in the same manner as the steering wire lumens 86a and 86b and the inlets 88a and 88b would simply extend through the wall of the distal member 18' to the proximal ends of the channels. Guide coils, or other tubular members through which the steering wires 52a and 52b pass, would be positioned within the channels. The electrodes 20 would be placed over the channels and guide coils.

III. Electrodes, Temperature Sensing and Power Control

In each of the preferred embodiments, the operative elements are a plurality of spaced electrodes 20. However, other operative elements, such as lumens for chemical ablation, laser arrays, ultrasonic transducers, microwave electrodes, and ohmically heated hot wires, and such devices may be substituted for the electrodes.

The spaced electrodes 20 are preferably in the form of wound, spiral coils. The coils are made of electrically conducting material, like copper alloy, platinum, or stainless steel, or compositions such as drawn-filled tubing (e.g. a

copper core with a platinum jacket). The electrically conducting material of the coils can be further coated with platinum-iridium or gold to improve its conduction properties and biocompatibility. A preferred coil electrode is disclosed in U.S. Patent No. 5,797,905. The electrodes 20 are electrically coupled to individual wires (not shown) to conduct coagulating energy to them. The wires are passed in conventional fashion through a lumen extending through the associated catheter body into a PC board in the catheter handle, where they are electrically coupled to a connector 76 that is received in a port on the handle. A connector 78 may be plugged into a source of RF coagulation energy and/or an electrophysiology recording system for mapping.

As an alternative, the electrodes may be in the form of solid rings of conductive material, like platinum, or can comprise a conductive material, like platinum-iridium or gold, coated upon the device using conventional coating techniques or an ion beam assisted deposition (IBAD) process. For better adherence, an undercoating of nickel or titanium can be applied. The electrodes can also be in the form of helical ribbons. The electrodes can also be formed with a conductive ink compound that is pad printed onto a non-conductive tubular body. A preferred conductive ink compound is a silver-based flexible adhesive conductive ink (polyurethane binder), however other metal-based adhesive conductive inks such as platinum-based, gold-based, copper-based, etc., may also be used to form electrodes. Such inks are more flexible than epoxy-based inks.

The flexible electrodes 20 are preferably about 4 mm to about 20 mm in length. In the preferred embodiment, the electrodes are 12.5 mm in length with 1 mm to 3 mm spacing, which will result in the creation of continuous lesion patterns in tissue when coagulation energy is applied simultaneously to adjacent electrodes. For rigid electrodes, the length of the each electrode can vary from about 2 mm to about 10 mm. Using multiple rigid electrodes longer than about 10 mm each adversely effects the overall flexibility of the device, while electrodes having lengths of less than about 2 mm do not consistently form the desired continuous lesion patterns.

The portion of the electrodes 20 that are not intended to contact tissue (and be exposed to the blood pool) may be masked through a variety of techniques with a material that is preferably electrically and thermally insulating. This prevents the transmission of coagulation energy directly into the blood pool and directs the energy directly toward and into the tissue. For example, a layer of UV adhesive (or another adhesive) may be painted on preselected portions of the electrodes to insulate the portions of the electrodes not intended to contact tissue. Deposition techniques may also be implemented to position a conductive surface only on those portions of the assembly intended to contact tissue. Alternatively, a coating may be formed by dipping the electrodes in PTFE material.

The electrodes may be operated in a uni-polar mode, in which the soft tissue coagulation energy emitted by the electrodes is returned through an indifferent patch electrode (not shown) externally attached to the skin of the patient. Alternatively, the electrodes may be operated in a bi-polar mode, in which energy emitted by one or more electrodes is returned through other electrodes. The amount of power required to coagulate tissue ranges from 5 to 150 w.

As illustrated for example in Figure 4, a plurality of temperature sensors 80, such as thermocouples or thermistors, may be located on, under, abutting the longitudinal end edges of, or in between, the electrodes 20. Preferably, the temperature sensors 80 are located at the longitudinal edges of the electrodes 20. In some embodiments, a reference thermocouple 82 may also be provided. For temperature control purposes, signals from the temperature sensors are transmitted to the source of coagulation energy by way of wires (not shown) that are also connected to the aforementioned PC board in the catheter handle. Suitable temperature sensors and controllers which control power to electrodes based on a sensed temperature are disclosed in U.S. Patent Nos. 5,456,682, 5,582,609 and 5,755,715.

In those instances where the ultimate orientation of a catheter relative to tissue (i.e. which side faces the tissue) is unpredictable, such as when a catheter with a pull wire is used, the temperature sensors 80 may be located

on two sides of catheter, as illustrated in Figure 4. Alternatively, in those instances where the orientation is more predictable, such as when the catheter is secured to the distal end of the sheath, the temperature sensors may all be located on the same side of the catheter, as illustrated in Figure 10. Here, the temperature sensors will be preferably located within a linear channel (not shown) that is formed in the distal member 18. The linear channel insures that the temperature sensors will directly face the tissue and be arranged in linear fashion. Such an arrangement results in more accurate temperature readings which, in turn, results in better temperature control. As such, the actual tissue temperature will more accurately correspond to the temperature set by the physician on the power control device, thereby providing the physician with better control of the lesion creation process and reducing the likelihood that embolic materials will be formed. Such a channel may be employed in conjunction with any of the electrode (or other operative element) supporting structures disclosed herein.

The electrodes 20 and temperature sensors 80 can include a porous material coating, which transmits coagulation energy through an electrified ionic medium. For example, as disclosed in U.S. Patent No. 5,991,650, electrodes and temperature sensors may be coated with regenerated cellulose, hydrogel or plastic having electrically conductive components. With respect to regenerated cellulose, the coating acts as a mechanical barrier between the surgical device components, such as electrodes, preventing ingress of blood cells, infectious agents, such as viruses and bacteria, and large biological molecules such as proteins, while providing electrical contact to the human body. The regenerated cellulose coating also acts as a biocompatible barrier between the device components and the human body, whereby the components can now be made from materials that are somewhat toxic (such as silver or copper).

Although the present inventions have been described in terms of the preferred embodiments above, numerous modifications and/or additions to the above-described preferred embodiments would be readily apparent to one skilled in the art. It is intended that the scope of the present inventions extend

to all such modifications and/or additions and that the scope of the present inventions is limited solely by the claims set forth below.

I claim:

1 1. A probe for use with an outer member including a wall defining
2 an interior bore, the probe comprising:

3 an elongate body, defining a distal region, a distal end, a
4 proximal region and an interior, adapted to be carried within the outer member
5 interior bore;

6 at least one operative element supported on the distal region of
7 the elongate body;

8 a control element defining a distal portion associated with the
9 distal end of the elongate body and a proximal portion extending along the
10 exterior of the elongate body toward the proximal region of the elongate body;
11 and

12 a steering element secured to the distal portion of the elongate
13 body and extending within the interior of the elongate body to the proximal
14 region of the elongate body.

1 2. A probe as claimed in claim 1, wherein the steering element
2 comprises a pair of steering elements.

1 3. A probe as claimed in claim 1, wherein the elongate body
2 comprises a catheter body.

1 4. A probe as claimed in claim 1, wherein at least the distal region
2 of the elongate body includes a flexible spline.

1 5. A probe as claimed in claim 4, wherein the flexible spline
2 comprises a solid core wire.

1 6. A probe as claimed in claim 4, wherein the flexible spline defines
2 a substantially circular cross sectional shape over a substantial portion thereof

3 and a substantially flat cross sectional shape over a relatively small portion
4 thereof.

1 7. A probe as claimed in claim 4, wherein the steering element is
2 fixedly secured to the flexible spline.

1 8. A probe as claimed in claim 1, wherein the operative element
2 comprises an electrode.

1 9. A probe as claimed in claim 1, wherein the proximal region of
2 the elongate body is relatively long and stiff and the distal region of the
3 elongate body is relatively short and flexible.

1 10. A probe as claimed in claim 1, wherein the control element
2 comprises a pull wire.

1 11. A probe for use with an outer member including a wall defining
2 an interior bore and a distal end, the probe comprising:

3 an elongate body, defining a distal region, a distal end, a
4 proximal region and an interior, adapted to be carried within the outer member
5 interior bore;

6 at least one operative element supported on the distal region of
7 the elongate body;

8 a connector adapted to connect the distal end of the elongate
9 body to the distal end of the outer member; and

10 a steering element secured to the distal portion of the elongate
11 body and extending within the interior of the elongate body to the proximal
12 region of the elongate body.

1 12. A probe as claimed in claim 11, wherein the steering element
2 comprises a pair of steering elements.

1 13. A probe as claimed in claim 11, wherein the elongate body
2 comprises a catheter body.

1 14. A probe as claimed in claim 11, wherein at least the distal region
2 of the elongate body includes a flexible spline.

1 15. A probe as claimed in claim 14, wherein the flexible spline
2 comprises a solid core wire.

1 16. A probe as claimed in claim 14, wherein the flexible spline
2 defines a substantially circular cross sectional shape over a substantial
3 portion thereof and a substantially flat cross sectional shape over a relatively
4 small portion thereof.

1 17. A probe as claimed in claim 14, wherein the steering element is
2 fixedly secured to the flexible spline.

1 18. A probe as claimed in claim 11, wherein the operative element
2 comprises an electrode.

1 19. A probe as claimed in claim 11, wherein the proximal region of
2 the elongate body is relatively long and stiff and the distal region of the
3 elongate body is relatively short and flexible.

1 20. A probe as claimed in claim 11, wherein the connector is integral
2 with the outer member.

1 21. A probe, comprising:
2 an elongate body defining a distal region and an interior;
3 a loop structure defining an interior and associated with the
4 distal region of the elongate body;
5 at least one operative element supported on the loop structure;
6 and

7 a steering element secured to the interior of the loop structure
8 and extending through the interior of the loop structure and the interior of the
9 elongate body to the proximal region of the elongate body.

1 22. A probe as claimed in claim 21, wherein the steering element
2 comprises a pair of steering elements.

1 23. A probe as claimed in claim 21, wherein the elongate body
2 comprises a catheter body.

1 24. A probe as claimed in claim 21, wherein at least the distal region
2 of the elongate body includes a flexible spline.

1 25. A probe as claimed in claim 24, wherein the flexible spline
2 comprises a solid core wire.

1 26. A probe as claimed in claim 24, wherein the flexible spline
2 defines a substantially circular cross sectional shape over a substantial
3 portion thereof and a substantially flat cross sectional shape over a relatively
4 small portion thereof.

1 27. A probe as claimed in claim 24, wherein the steering element is
2 fixedly secured to the flexible spline.

1 28. A probe as claimed in claim 21, wherein the operative element
2 comprises an electrode.

1 29. A probe as claimed in claim 21, wherein the proximal region of
2 the elongate body is relatively long and stiff and the distal region of the
3 elongate body is relatively short and flexible.

1 30. A probe as claimed in claim 21, further comprising:
2 a control element defining a distal portion associated with the
3 loop structure and a proximal portion extending along the exterior of the
4 elongate body toward the proximal region of the elongate body.

1 31. A probe, comprising:
2 an elongate body defining a distal region and a proximal region;
3 at least one operative element supported on the distal region of
4 the elongate body; and
5 a steering element secured at a first side of the distal region of
6 the elongate body and extending to a second side of the distal region opposite
7 the first side of the distal region and from the second side of the distal region
8 to the proximal region of the elongate body.

1 32. A probe as claimed in claim 31, wherein the distal portion of the
2 elongate body defines a steering wire lumen extending from the first side to
3 the second side.

1 33. A probe as claimed in claim 31, wherein the first side is offset
2 from the second side by 180 degrees.

1 34. A probe as claimed in claim 31, wherein the steering wire is
2 secured to the at least one operative element.

FIG. 1

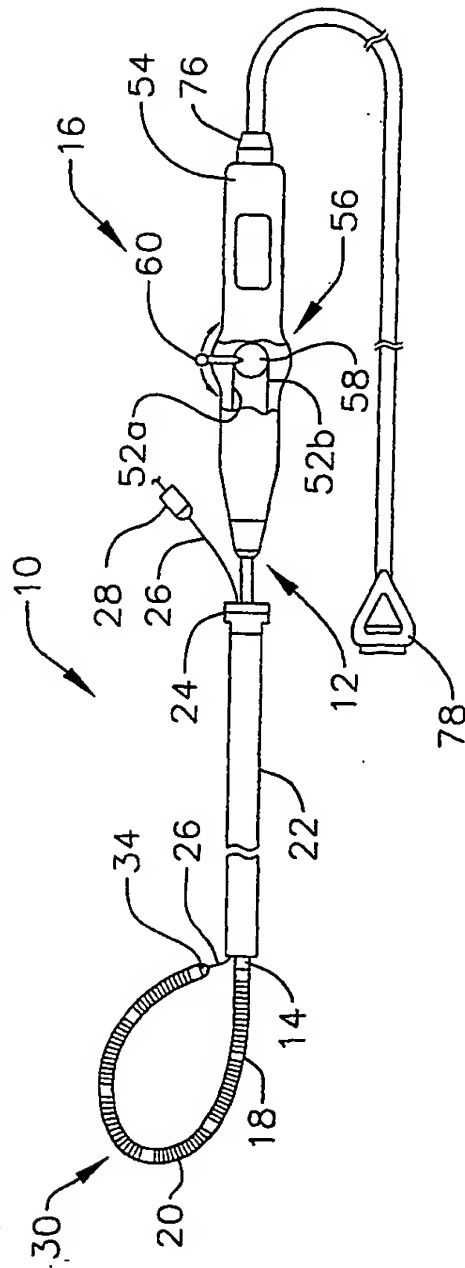


FIG. 2

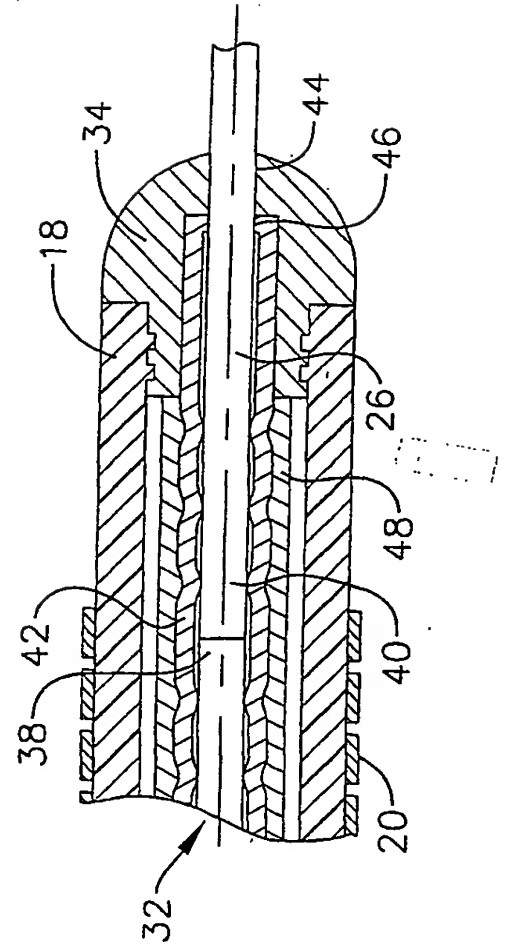


FIG. 3

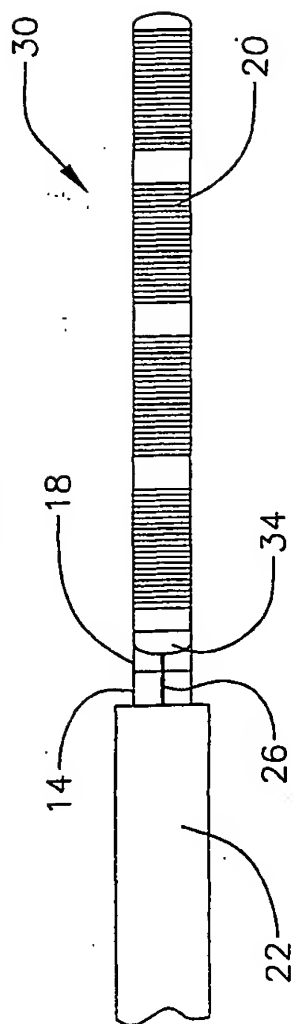


FIG. 4

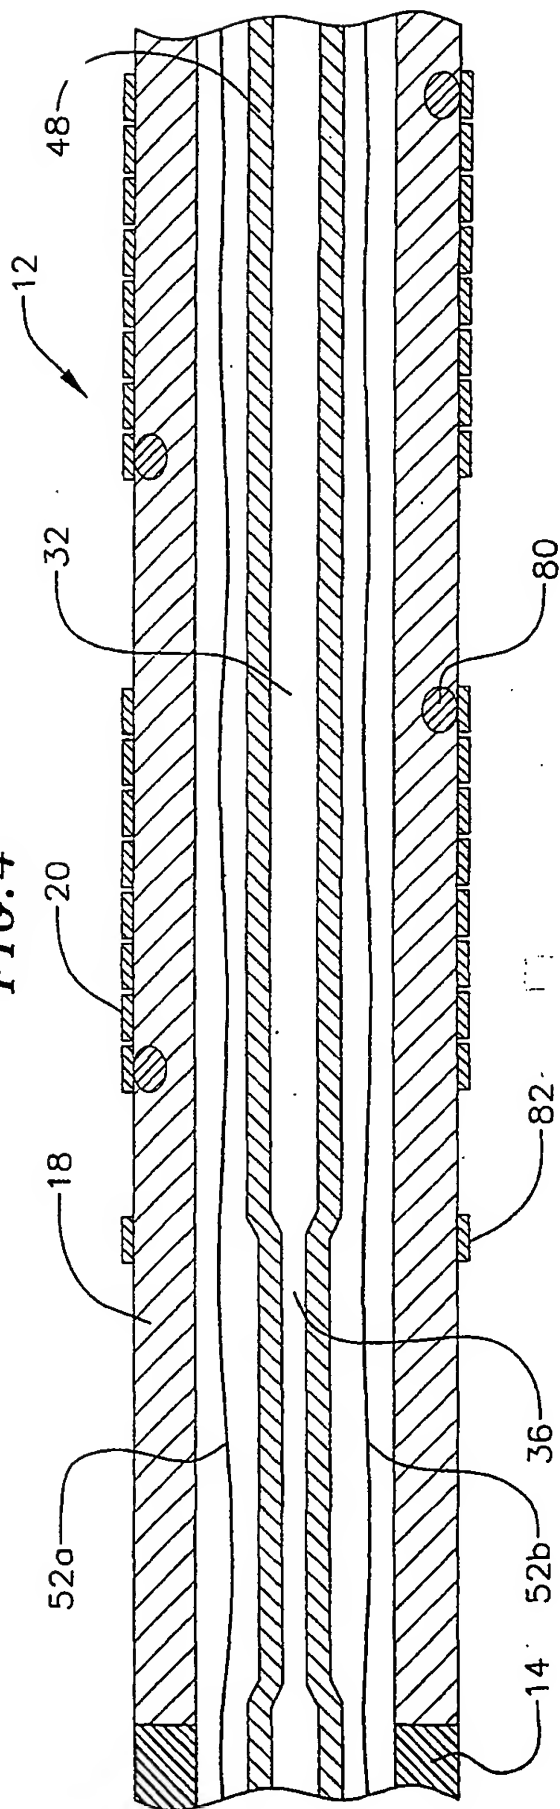


FIG. 5

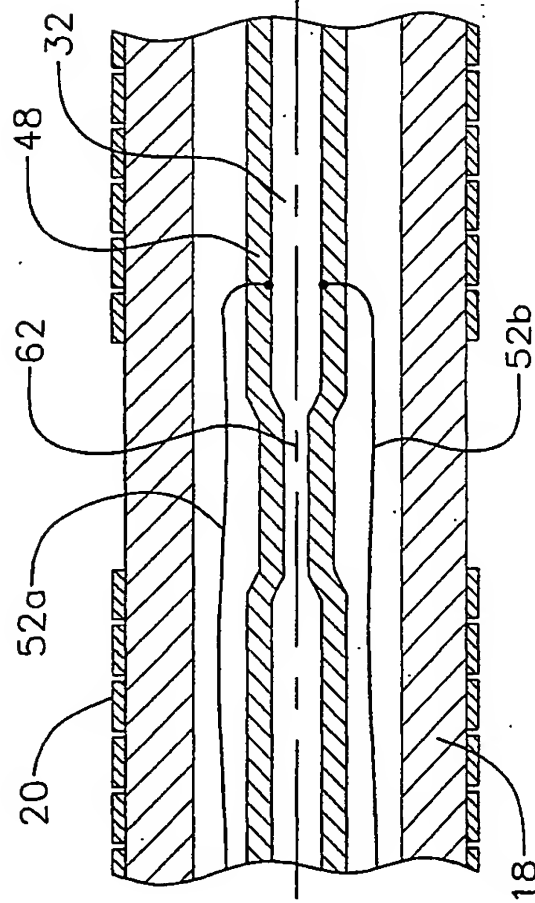


FIG. 6

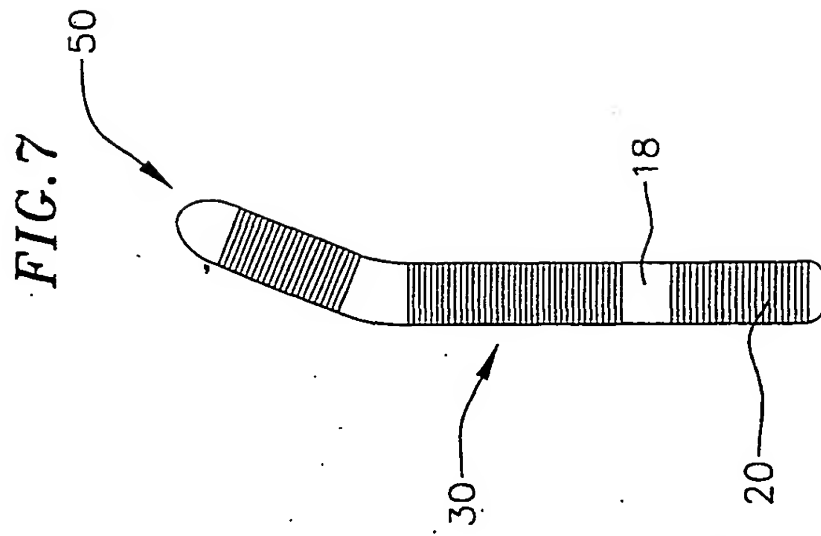
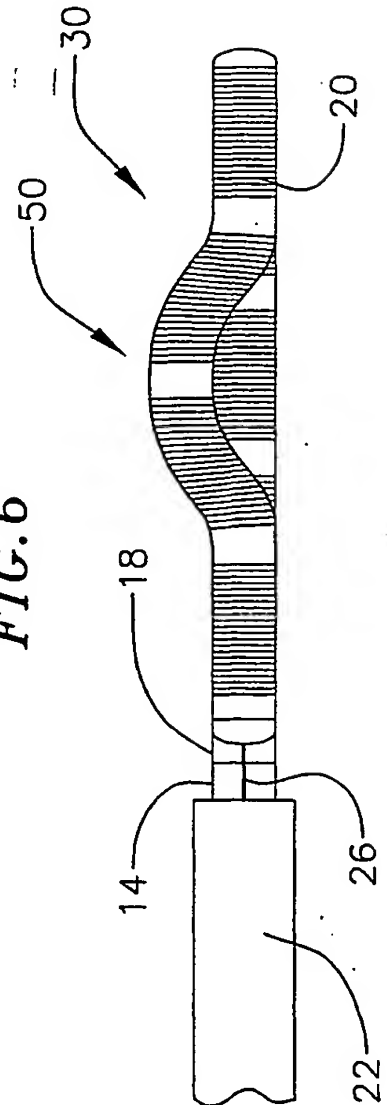


FIG. 9

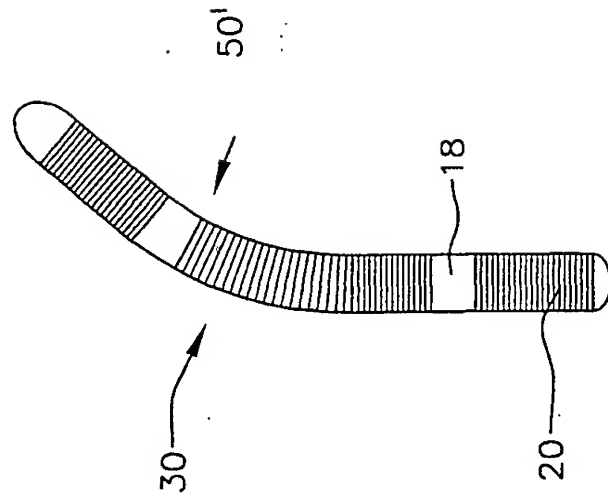


FIG. 8





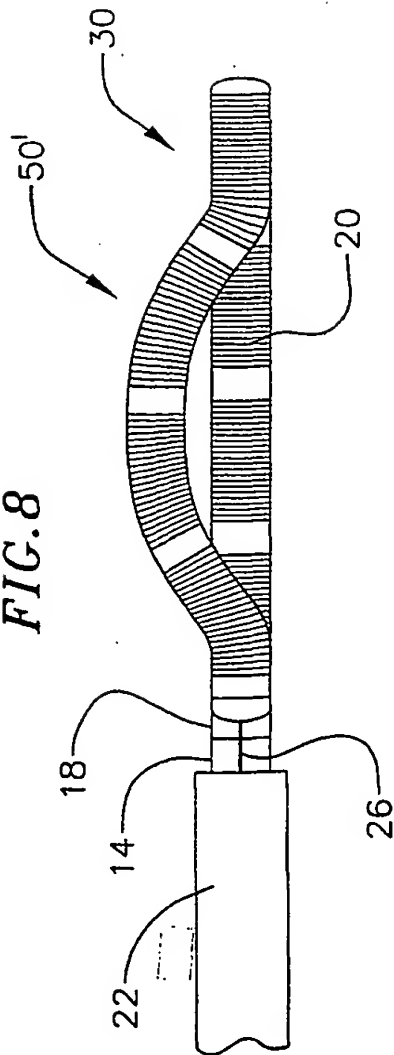


FIG. 10

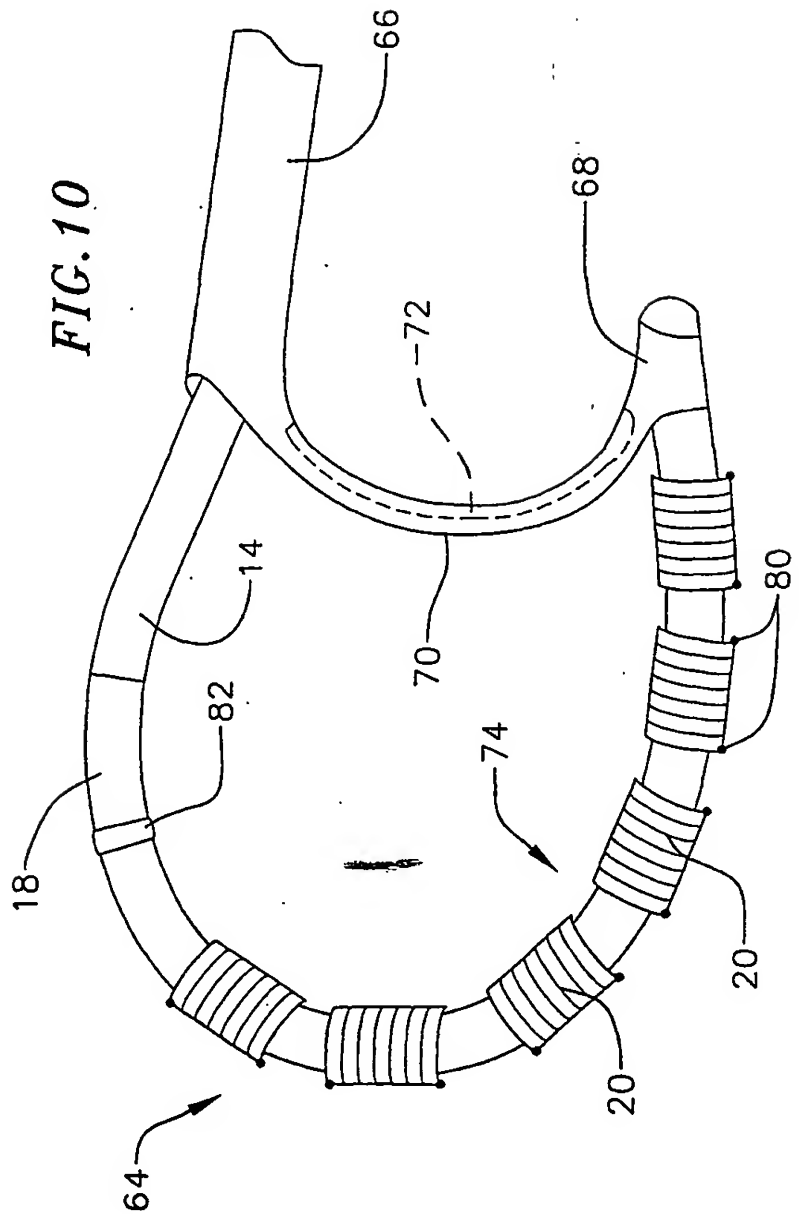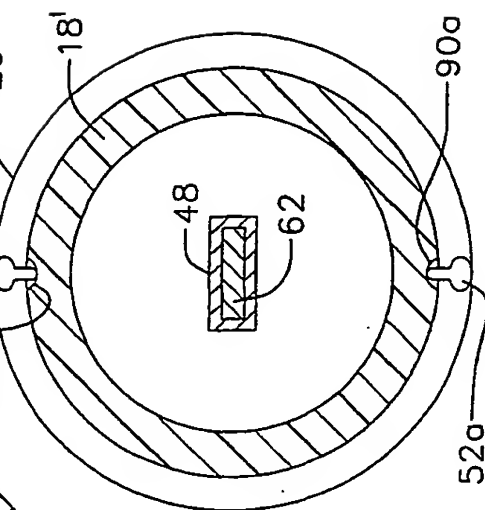

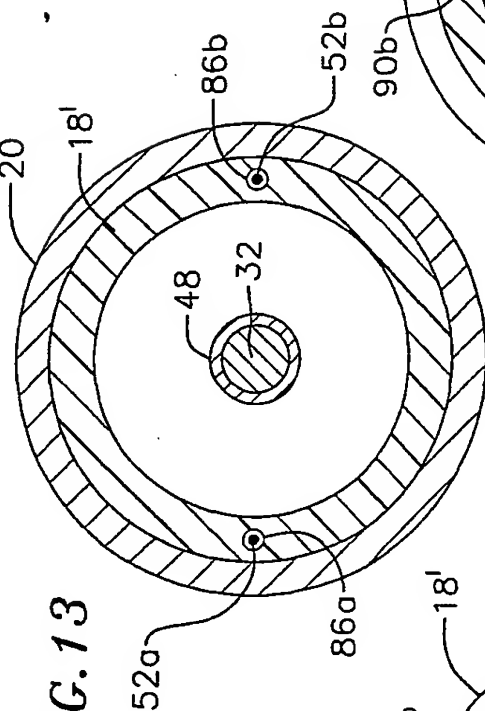

(19) World Intellectual Property Organization
International Bureau

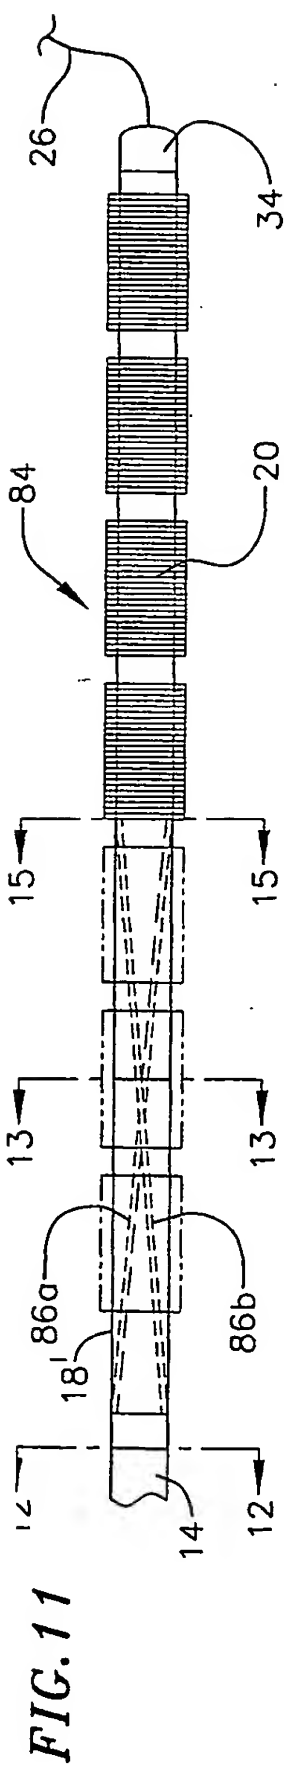

(43) International Publication Date
16 May 2002 (16.05.2002)

PCT

(10) International Publication Number
WO 02/038052 A3

(51) International Patent Classification⁷: **A61B 18/14**

(21) International Application Number: PCT/EP01/12243

(22) International Filing Date: 23 October 2001 (23.10.2001)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
09/709,087 10 November 2000 (10.11.2000) US

(71) Applicant (*for all designated States except US*): **BOSTON SCIENTIFIC LIMITED** [B/BB], Financial Services Centre, P.O. Box 111 Bishop's Court Hill, St. Michael (BB).

(72) Inventors: and

(75) Inventors/Applicants (*for US only*): **JENKINS, Thomas, R.** [US/US], 3750 McClelland Ave., Oakland, CA 94619 (US); **SWANSON, David, K.** [US/US], 1458 Ridgeley Drive, Campbell, CA 95008 (US)

(74) Agent: **VIERING, JENTSCHURA & PARTNER**, Steinsdorfstr. 6, 80335 Munich (DE).

(81) Designated States (*national*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, PH, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, TZ, UA, UG, US, UZ, VN, YU, ZA, ZW.

(84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).


Published:

— with international search report

(88) Date of publication of the international search report:
31 October 2002

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(54) Title: **STEERABLE LOOP STRUCTURE**

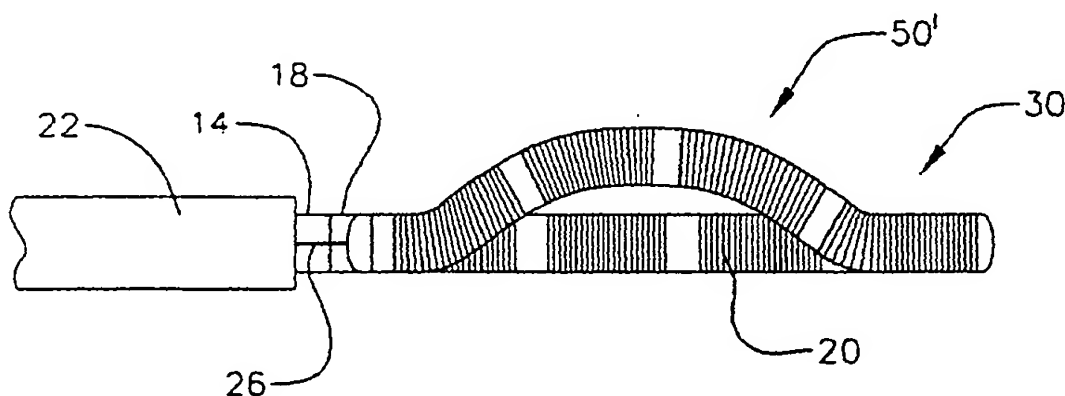

(57) Abstract: A probe that includes an elongate body (12) and a steerable loop structure (30, 74) that supports electrodes (20) or other operative elements against the body tissue.



WO 02/038052 A3

A. CLASSIFICATION OF SUBJECT MATTER IPC 7 A61B18/14		
According to International Patent Classification (IPC) or to both national classification and IPC		
B. FIELDS SEARCHED Minimum documentation searched (classification system followed by classification symbols) IPC 7 A61B		
Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched		
Electronic data base consulted during the international search (name of data base and, where practical, search terms used) EPO-Internal		
C. DOCUMENTS CONSIDERED TO BE RELEVANT		
Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	WO 99 05971 A (CARDIAC PATHWAYS CORP) 11 February 1999 (1999-02-11) page 8, paragraph 2; figure 36B page 41, paragraph 5Y page 17, paragraph 4 ---	1-4
Y	US 5 730 127 A (AVITALL BOAZ) 24 March 1998 (1998-03-24) column 14, line 55-67; figures 36,30 ---	1,3
Y	US 5 871 523 A (FLEISCHMAN SIDNEY D ET AL) 16 February 1999 (1999-02-16) column 9, line 10-20; figure 16 ---	1,2,4
A	US 5 656 029 A (GLYNN BRIAN A ET AL) 12 August 1997 (1997-08-12) figures 8A,8B,8C -----	6
<div style="display: flex; justify-content: space-between;"> <input type="checkbox"/> Further documents are listed in the continuation of box C. <input checked="" type="checkbox"/> Patent family members are listed in annex. </div>		
<div style="display: flex;"> <div style="flex: 1;"> <p>* Special categories of cited documents :</p> <p>"A" document defining the general state of the art which is not considered to be of particular relevance</p> <p>"E" earlier document but published on or after the international filing date</p> <p>"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)</p> <p>"O" document referring to an oral disclosure, use, exhibition or other means</p> <p>"P" document published prior to the international filing date but later than the priority date claimed</p> </div> <div style="flex: 1;"> <p>"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention</p> <p>"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone</p> <p>"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art</p> <p>"&" document member of the same patent family</p> </div> </div>		
Date of the actual completion of the international search <div style="text-align: center; font-size: 1.2em;">12 March 2002</div>	Date of mailing of the international search report <div style="text-align: center; font-size: 1.2em;">10.05.02</div>	
Name and mailing address of the ISA European Patent Office, P.B. 5818 Patentlaan 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-2040, Tx. 31 651 epo nl, Fax: (+31-70) 340-3016	Authorized officer <div style="text-align: center; font-size: 1.2em;">PAPONE, F</div>	

INTERNATIONAL SEARCH REPORT

international application No.
PCT/EP 01/12243**Box I Observations where certain claims were found unsearchable (Continuation of item 1 of first sheet)**

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☐ Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:
2. ☐ Claims Nos.:
because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box II Observations where unity of invention is lacking (Continuation of item 2 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

see additional sheet

1. ☐ As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☒ No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

1-10

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest.
- ☐ No protest accompanied the payment of additional search fees.

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210

This International Searching Authority found multiple (groups of) inventions in this international application, as follows:

1. Claims: 1-10

Probe with sheath and elongate body(cath)having a steerable distal portion

2. Claims: 11-20

Probe with sheath and elongate body(cath)having a steerable distal portion, with connector (tether) between the two distal portions

3. Claims: 21-30

Probe with sheath and elongate body(cath)having a steerable distal portion this last one in the form of a loop

4. Claims: 31-34

Probe with sheath and elongate body(cath)having a steerable distal portion, wherein the shape wires cross sides along distal end.

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
WO 9905971	A	11-02-1999	WO 9905971 A1	11-02-1999
			US 6216027 B1	10-04-2001

US 5730127	A	24-03-1998	US 5687723 A	18-11-1997
			US 5487385 A	30-01-1996
			US 6138043 A	24-10-2000
			US 6308091 B1	23-10-2001
			US 2002002329 A1	03-01-2002
			US 5842984 A	01-12-1998
			US 5921924 A	13-07-1999
			AU 685559 B2	22-01-1998
			AU 1265495 A	19-06-1995
			CA 2177982 A1	08-06-1995
			EP 0731665 A1	18-09-1996
			JP 3237849 B2	10-12-2001
			JP 9506017 T	17-06-1997
			WO 9515115 A1	08-06-1995

US 5871523	A	16-02-1999	US 5545193 A	13-08-1996
			CA 2174129 A1	20-04-1995
			CA 2174131 A1	20-04-1995
			EP 0754075 A1	22-01-1997
			EP 0723469 A1	31-07-1996
			JP 9509069 T	16-09-1997
			JP 10507373 T	21-07-1998
			WO 9510318 A1	20-04-1995
			WO 9510319 A1	20-04-1995
			WO 9510236 A1	20-04-1995
			WO 9510321 A1	20-04-1995
			WO 9510327 A1	20-04-1995
			US 5582609 A	10-12-1996
			US 6106522 A	22-08-2000
			US 6171306 B1	09-01-2001
			US 6129724 A	10-10-2000

US 5656029	A	12-08-1997	US 5478330 A	26-12-1995
			US 5391147 A	21-02-1995
			US 5389073 A	14-02-1995
			AU 675088 B2	23-01-1997
			AU 5183393 A	16-06-1994
			CA 2109980 A1	02-06-1994
			EP 0600676 A2	08-06-1994
			JP 2644434 B2	25-08-1997
			JP 6261952 A	20-09-1994
			US 5588964 A	31-12-1996
			US 5533967 A	09-07-1996

THIS PAGE BLANK (USPTO)